









CELLAVISION DIFFERENTIAL

Collected on April 3, 2024 6:07 AM

automated digital morphology of WBC

Lab tests - Blood (Blood, Venous)

Results New

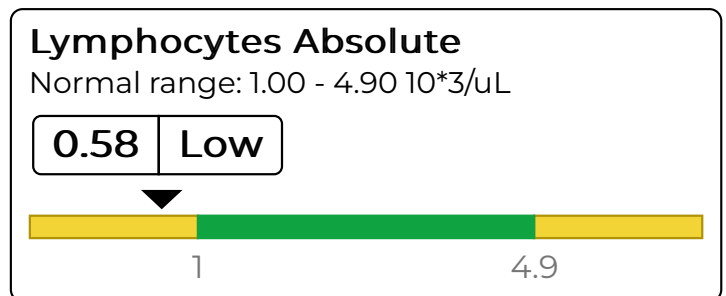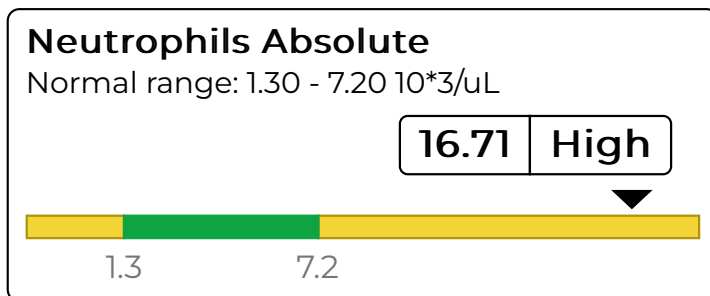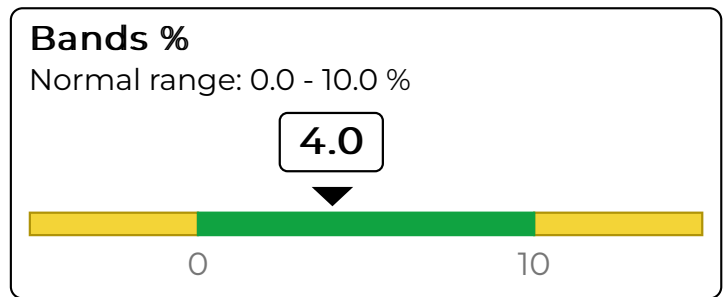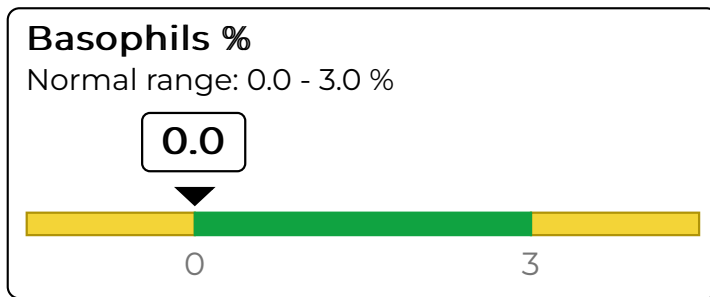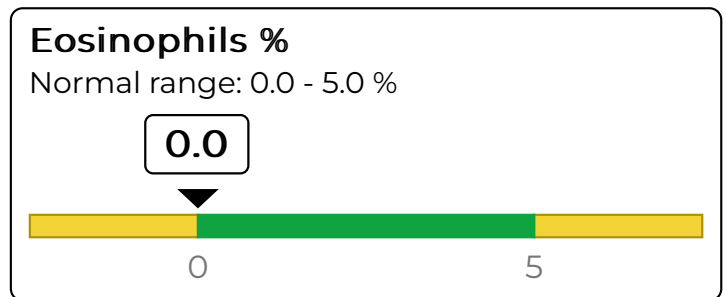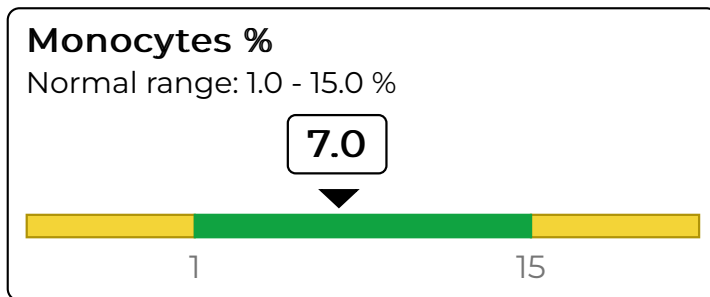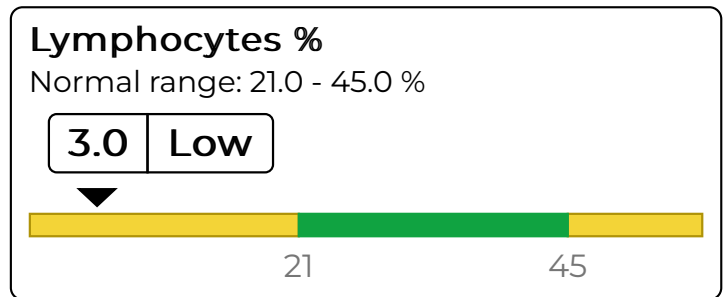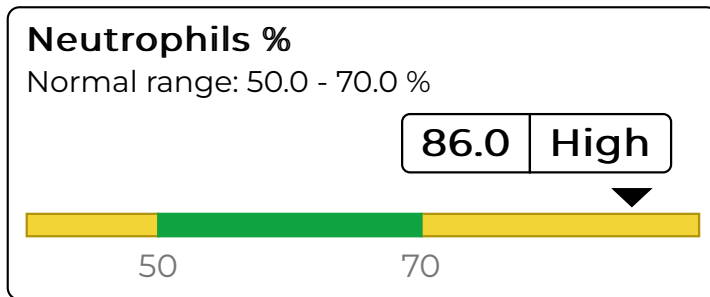

Monocytes Absolute

Normal range: 0.30 - 1.00 $10^3/\mu\text{L}$

1.36 High



Eosinophils Absolute

Normal range: 0.00 - 0.40 $10^3/\mu\text{L}$

0.00



Basophil Absolute

Normal range: 0.00 - 0.30 $10^3/\mu\text{L}$

0.00



Bands Absolute

$10^3/\mu\text{L}$


Value

0.78

Neutrophils Absolute (Segs+Bands)

Normal range: 1.30 - 7.20 $10^3/\mu\text{L}$

17.49 High



Ordering provider: Jigna Hitesh Shah, MD

Collection date: April 3, 2024 6:07 AM

Result date: April 3, 2024 12:44 PM

Result status: Final

Resulting lab:

ADVENTHEALTH LAB WATERMAN

1000 Waterman Way

TAVARES FL 32778

352-253-3375

Deborah Lynn Zeagler, MD (Lab director)

10D0273538 (CLIA #)